



GIMA

PROFESSIONAL MEDICAL PRODUCTS

Gima S.p.A.
Via Marconi, 1 - 20060 Gessate (MI) Italy
gima@gimaitaly.com - export@gimaitaly.com
www.gimaitaly.com

SP-10 POCKET SPIROMETER

User manual



ATTENTION: The operators must carefully read and completely understand the present manual before using the product.

REF 33536




CONTEC MEDICAL SYSTEMS CO., LTD
ADD: No 112 Qinhuang West Street,
Economic & Technical Development Zone,
Qinhuangdao, Hebei Province, 066004,
PEOPLE'S REPUBLIC OF CHINA
Made in China



Shanghai International Holding Corp. GmbH (Europe)
Eiffestrasse 80, 20537 Hamburg, Germany

Importato e distribuito da:
Gima S.p.A. - Via Marconi, 1 - 20060 Gessate (MI) Italy

CE 0123





Dear users, thank you very much for purchasing the SPIROMETER.

Please read the User Manual carefully before using this product. The User Manual which describes the operating procedures should be followed strictly. Failure to follow the User Manual may cause measuring abnormality, equipment damage and human injury. The manufacturer is NOT responsible for the safety, reliability and performance issues and any monitoring abnormality, human injury and equipment damage due to users' negligence of the operation instructions. The manufacturer's warranty service does not cover such faults.

Owing to the forthcoming renovation, the specific products you received may not be totally in accordance with the description of this User Manual. We would sincerely regret for that.

This product is medical device, which can be used repeatedly.

WARNING:

- For accuracy, it is recommended that the SPIROMETER should not be tested on the same testee for more than 5 times.
- The testee should breathe out all air during testing, don't exchange air or cough.
- Don't use the device in environment with lower temperature.
- Automatic power off when there is no operation in one minute.
- Please refer to the correlative literature about the clinical restrictions and caution.
- This device is not intended for treatment.

Our company reserves the final elucidative right.



Contents

| | |
|--|-----------|
| Chapter 1 Safety | 5 |
| 1.1 Instructions for Safe Operations | 5 |
| 1.2 Warning..... | 5 |
| 1.3 Attention..... | 6 |
| 1.4 Contraindication..... | 6 |
| 1.5 EMC declaration | 7 |
| Chapter 2 Overview | 8 |
| 2.1 Features | 8 |
| 2.2 Major Applications and Scope..... | 8 |
| 2.3 Environment Requirements..... | 9 |
| Chapter 3 Principle | 9 |
| Chapter 4 Technical Specifications..... | 9 |
| 4.1 Main Performance..... | 9 |
| 4.2 Main Parameters..... | 10 |
| Chapter 5 Installation | 11 |
| 5.1 View of the Front Panel..... | 11 |
| 5.2 Assembly and disassembly | 11 |
| 5.3 Accessories..... | 12 |
| Chapter 6 Operating Guide | 12 |
| 6.1 How to use..... | 12 |
| 6.1.1 Power on/off | 12 |
| 6.1.2 Measurement | 12 |
| 6.1.3 Main Interface | 13 |
| 6.1.4 Menu..... | 15 |
| 6.1.5 Repeated measure..... | 25 |
| 6.1.6 Charge | 26 |
| 6.1.7 Upload Data..... | 26 |



| | |
|--|-----------|
| 6.2 Attention..... | 27 |
| Chapter 7 Maintenance,Transportation and Storage..... | 27 |
| 7.1 Cleaning and Disinfection | 27 |
| 7.2 Maintenance | 27 |
| 7.3 Transportation and Storage | 28 |
| Chapter 8 Troubleshooting | 28 |
| Chapter 9 Key of Symbols | 30 |
| Chapter 10 Parameter Introduction..... | 31 |
| Appendix I | 32 |



Chapter 1

SAFETY

1.1 Instructions for Safe Operations

- Check the main unit and all accessories periodically to make sure that there is no visible damage that may affect patient's safety and monitoring performance. It is recommended that the device should be inspected weekly at least. When there is obvious damage, stop using the device.
- All maintenance must be performed by qualified service engineers ONLY. Users are not permitted to maintain it by themselves.
- The SPIROMETER cannot be used together with devices not specified in User Manual. Only the accessory that is appointed or recommendatory by manufacture can be used with this device.
- This product has been calibrated before leaving factory.

1.2 Warning

- ⚠ Explosive hazard—DO NOT use the SPIROMETER in the environment with tinder such as anesthetic.
- ⚠ Please check the packing before use to make sure the device and accessories are totally in accordance with the packing list, or else the device may have the possibility of working abnormally.
- ⚠ Don't use the device in environment with strong electromagnetic interference, direct breeze source, cold source and hot source.
- ⚠ Portable or mobile RF equipment with strong electromagnetic interference may influence the accuracy of this device.
- ⚠ Improper disposal of device and its accessories and packing (include mouthpiece, plastic bags, foams and paper boxes) may cause environment pollution, please follow the local laws and regulations.
- ⚠ Please choose the accessories which are appointed or recommended by the manufacturer for avoiding device damage.
- ⚠ Don't use the device with the turbine of the same kind product.
- ⚠ DO NOT use the device when it is under charging state.



- The red and green indicators are all highlight in charging state, the red indicator goes out when the charge has finished.

1.3 Attention

- Keep the SPIROMETER away from dust, vibration, corrosive substances, tinder, high temperature and moisture.
- If the SPIROMETER gets wet, please stop operation.
- When it is carried from cold environment to warm or humid environment, please do not use it immediately.
- DO NOT operate button on front panel with sharp things.
- High temperature or high pressure steam disinfection to the device is not permitted. Refer to User Manual in the relative chapter (7.1) for cleaning and disinfection.
- Do not have the SPIROMETER immersed in liquid. When it needs cleaning, please wipe its surface with medical alcohol by soft material. Do not spray any liquid on the device directly.
- When cleaning the device with water, the temperature should be lower than 60°C.
- The display period of data is less than 5 seconds, which is changeable according to the end rate.
- When data can't be displayed at all times or other cases happened during testing, press "repeated measure" key to remeasure, or power off to restart.
- The device has normal life for three years since the first electrified use.
- When the data goes beyond the limits, the main screen shows "Error!".
- The device doesn't suit all users, if you can't get good measurement data, please stop using it.
- The device needs to be calibrated once per year or less.
- The device is forced SPIROMETER, according to the User Manual to use right to gain best result.

1.4 Contraindication

1.4.1 Absolute contraindication

- The one with MI or shock in recent 3 months;
- The one with serious cardiac function unstable or angina pectoris in recent 4 weeks;

- ⚠ The one with massive hemoptysis in recent 4 weeks;
- ⚠ The one who needs medication in epileptic seizure;
- ⚠ The one with uncontrolled hypertensive disease (SYS>200mmHg, DIA>100mmHg);
- ⚠ The one with aortic aneurysm;
- ⚠ The one with serious hyperthyroidism.

1.4.2 Relative contraindication

- ⚠ Heart rate >120 beats/min;
- ⚠ The one with pneumothorax or giant pulmonary bulla and not plan for surgical treatment;
- ⚠ The one with pregnancy;
- ⚠ The one with tympanic membrane perforation (need to block the ear canal of affected side before taking measurement);
- ⚠ The one with RTI recently (less than 4 weeks);
- ⚠ The one with hypoimmunity.

Patients of respiratory communicable disease or infectious disease shall not take lung function examination in the acute stage. The one with low immunity is not appropriate to take the examination also. If it is necessary, disease control and protection shall be strictly followed.

1.5 EMC declaration

- ⚠ When this device is installed or putted into service, EMC should be paid more attention, as the portable and mobile RF communications equipment with higher EM interference can affect this device.
- ⚠ The internal components and cables should not be changed, as this may decreased IMMUNITY of the device.
- ⚠ The SPIROMETER should not be used adjacent to or stacked with other equipments.



Chapter 2

OVERVIEW

Forced Vital Capacity is the maximum expiration after taking a full breath, it's an important examination content in chest-lung disease and respiratory health, and it is indispensable testing project in modern Pulmonary inspection. At the same time, it has great significance in respiratory diseases, differential diagnosis, treatment evaluation and selection of surgical indications. Thus, with the rapid development of clinical respiratory physiology, clinical applications of lung capacity inspection are also gaining popularity.

The SPIROMETER is small in volume, low in power consumption, convenient in operation and portable. With high-definition display screen, the device is concise and fashion. It is only necessary for patient to breath in fully and seal the lips around the mouthpiece and blast the air out in best times for measure, then the display screen will directly show the Forced Vital Capacity (FVC), Forced Expired Volume in one second (FEV1), Peak Expiratory Flow (PEF) with the high veracity and repetition.

2.1 Features

- 1) Ultra-thin design, concise and fashion.
- 2) Small in volume, light in weight and convenient in carrying.
- 3) Low power consumption.
- 4) TFT display.
- 5) Reflect lung function by measuring FVC, FEV1, PEF etc.

2.2 Major Applications and Scope

The SPIROMETER is a hand-held equipment for examining lung function. The product is fit for hospital, clinique, family for ordinary test. It's only required that the user operates it according to user manual, no need for specialized training, so the operation of the device would be as simple and easy as possible.

2.3 Environment Requirements

Storage Environment:

Temperature: $-40^{\circ}\text{C}\sim+55^{\circ}\text{C}$

Relative humidity: $\leq 95\%$

Atmospheric pressure: 500hPa~1060hPa

Operating Environment:

Temperature: $+10^{\circ}\text{C}\sim+40^{\circ}\text{C}$

Relative Humidity: $\leq 80\%$

Atmospheric pressure: 700hPa~1060hPa

Chapter 3 PRINCIPLE

Firstly, testee deep inspires, then seals the lips around the mouthpiece and blasts all air out as forcefully as possible, the exhalant gas transforms to rotary airflow by turbine, then makes the blade rotate. The reception part of the infrared pair diodes (one is for infrared emission, the other is reception) towards to the blade is used for receiving the infrared ray, when the blade rotates, the received ray strength of the reception diode will be different as the difference of the blade angle, so form the various signal of same proportion in reception diode, which forms acquisition signal by SCM after processing. At last, various parameters to be measured formed from the information which were processed by the microprocessor, and displayed from the screen.

Chapter 4 TECHNICAL SPECIFICATIONS

4.1 Main Performance

- Forced Vital Capacity (FVC), Forced Expired Volume in one second (FEV1), the ratio of FEV1 and FVC (FEV1%),



Peak expiratory flow (PEF), 25% flow of the FVC (FEF25), 75% flow of the FVC (FEF75) and average flow between 25% and 75% of the FVC (FEF2575) can be measured. Besides, the testee condition can be shown by the ratio of the measured value and the predicted value.

- Flow rate-volume chart, volume-time chart display.
- Data memory, delete, upload and review.
- Trend chart display.
- Calibration.
- Information prompts when volume or flow goes beyond the limits.
- Automatic power off when there is no operation in one minute.
- Rechargeable lithium battery and with charging tips.
- Battery power display.

4.2 Main Parameters

Volume Range: 10L

Flow range: 0 L/s~16 L/s

Volume accuracy: $\pm 3\%$ or 0.05L (whichever is greater)

Flow accuracy: $\pm 5\%$ or 0.2L/s (whichever is greater)

Working current: 60mA

Power supply: DC3.7V 820mAh rechargeable lithium battery

Classification:

EMC: Group I Class B.

According to the MDD 93/42, the classification of this medical device: IIa.

The type of protection against electroshock: Internally powered equipment.

The degree of protection against electroshock: Type BF applied part .

International Protection: IPX0.

Chapter 5 INSTALLATION

5.1 View of the Front Panel

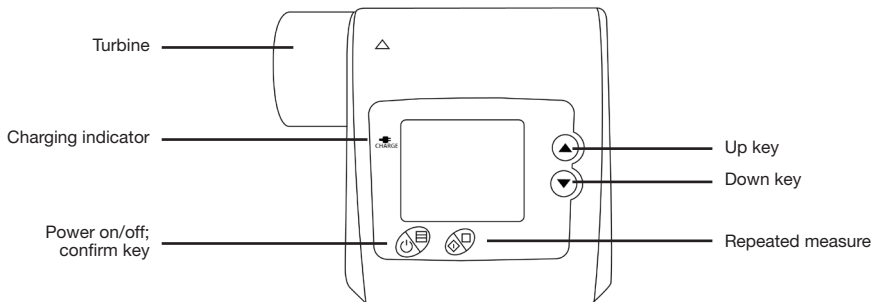


Figure 1 Front panel view

5.2 Assembly and disassembly

- 1) Turbine assembly: Hold the turbine, align the arrowhead of the turbine with the triangular shape on the shell, gently insert it to the bottom, counterclockwise rotate to lock it
- 2) Turbine disassembly: clockwise rotate the turbine, gently pull it out
- 3) Mouthpiece assembly: insert the mouthpiece into the turbine port directly



5.3 Accessories

- 1) A User Manual
- 2) A USB data line
- 3) A mouthpiece
- 4) A power adapter
- 5) A CD (PC software)
- 6) A nose clip (optional)

 Other type adapter should meet the following conditions: output voltage: DC 5V; output current $\geq 500\text{mA}$, the power adapter must meet the requirements of EN60601 related standards and have the CE mark.

Chapter 6 OPERATING GUIDE

6.1 How to use

6.1.1 Power on/off

1. After assembly, long press “power on” key to turn on the device.
2. When device is powered on, long press “power off” key to turn it off.

6.1.2 Measurement

1. The device is in [Selective interface] after turn on as shown in Fig.2, press “up” or “down” key to select “No”, then press “confirm” key to enter [Testing] interface as shown in Fig.3. (Note: If select “Yes”, it will enter [Personal information] interface to edit personal information, after exit, it will return to [Testing] interface.)
2. In [Testing] interface, breath in fully, seal the lips around the mouthpiece and blast all air out as forcefully as possible in a minimal amount of time, wait for a few seconds, the device will enter [Main parameter] interface as shown in Fig.4.

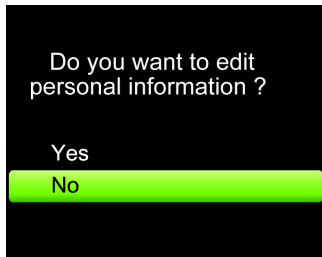


Figura 2 Interfaccia "Selective"

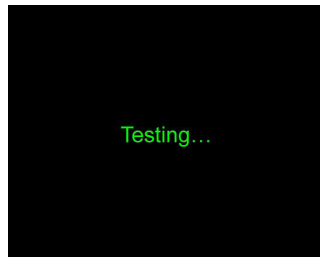


Figura 3 Interfaccia "Testing"

6.1.3 Main Interface

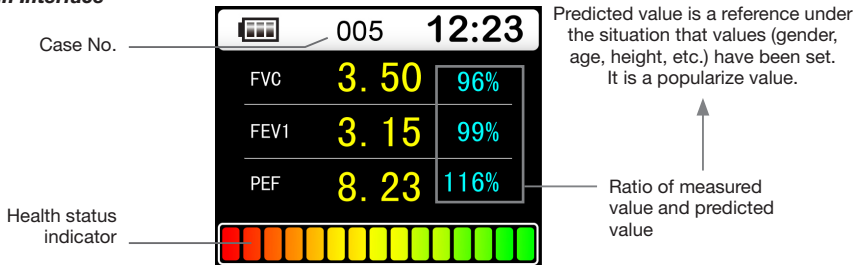


Figura 4 Interfaccia "Main parameter"



- a. **Main parameter interface:** display the ratio of predicted value and measured value of three main parameters. Ratio reflects health status, correct settings of personal information is the key to obtain accuracy ratio. Besides, this interface can also display battery status, time, case number and health status indicator, as shown in Fig.4.
- b. **Health status indicator:** indicate the ratio of measured value and the predicted value, display the testee health condition in image. I.e. Compare the measured value with the reference value in same situation. When the value is lower than 50%, only red indicator is displayed, which means testee should pay attention and go to hospital in time. When the value is in range from 50%-80%, red and yellow indicator are displayed, which means it should be noticed. When the value is higher than 80%, all red, yellow and green indicator are displayed, which means healthy. The determinate item of health status indicator is optional, it can be set in “Denote value” under “Date management”.
- c. **Other parameter interface:** display four parameters except the main parameter, as shown in Fig.5.
- d. Under [Main parameter] interface, press “Up” or “Down” key will enter [Other parameter] [Flow rate-volume chart] [Volume-time chart] in turn, as shown in Fig.5, 6, 7. The four interfaces above are [Main interface].

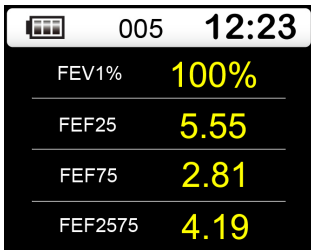


Figure 5 Other parameter interface

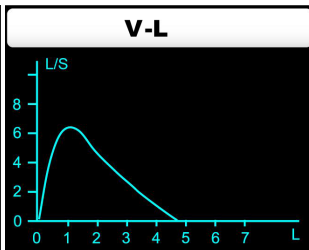


Figure 6 Flow rate-volume chart

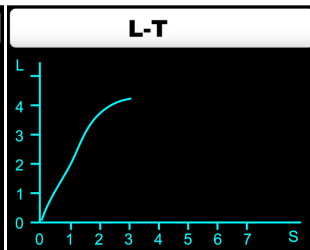


Figure 7 Volume-time chart

6.1.4 Menu

Under [Testing] or [Main interface], press confirm key to enter [Menu] interface as shown in Fig.8. Under the interface, functions such as modify personal information, data management, device setting, power off can be realized. Press “Up” or “Down” key to move the selection toolbar to the item that need to be modified, then press “Confirm” key to enter the sub-menu. See the following steps for details:

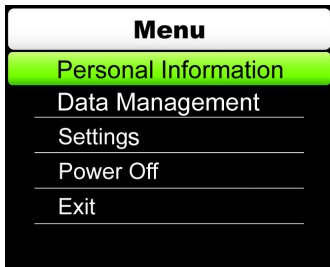


Figure 8 Menu interface

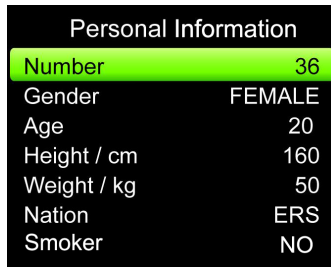


Figure 9 Personal information interface

a. PERSONAL INFORMATION

Under [Menu] interface, select “Personal information” to enter its interface as shown in Fig.9, in which user can edit patient information (Note: Under [Selective interface] as shown in Fig.2, if selected “Yes”, you can enter [Personal information] interface also.).

1. Case number

“Number” is the case number displayed at present. For example, if you are the 36th testee, the “Number” will be 36. Case number can increase automatically, no need to set manually.

2. Gender setting

Under [Personal information] interface, press “Up” or “Down” key to move the selection toolbar to “Gender”, then press “Confirm” key to select “female” or “male”.

3. Setting of age, height, weight

Under [Personal information], select “Age” to enter [Age edit] interface, as show in Fig.10. Press “Up” or “Down” key to change the value. At each pressing of “Up” or “Down” key, the value will plus or minus 1. When long press the “Up” or “Down” key, the value will increase or decrease continuously. Press “Confirm” key to back to [Personal information] interface.

The modification of “Height” and “Weight” is similar to the “Age”. In which, range of “Age” is 6~100 years old, range of “Height” is 80~240 cm, range of “Weight” is 15~250 kg.

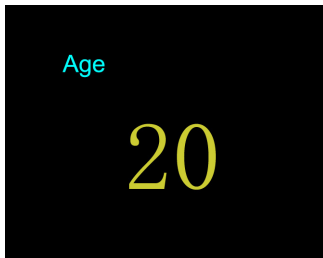


Figure 10 Age edit interface

4. Nation setting

The modification of “Nation” is similar to the “Gender”. The standard of predicted value can be set under “Nation” interface, which including ERS, KNUDSON and USA. ERS is the European standard, KNUDSON is the Asian standard, USA is the American standard.

5. Setting of smoker and drug

The modification of “Smoker” and “Drug” is similar to the “Gender”, in which patient information of smoker and drug can be modified.

For the display of screen is limited, the device won’t display all items at the same time. When selection toolbar moved to “Smoker”, press “Down” key, the item of “Drug” and “Exit” will appear, as shown in Fig. 11, 12.

6. Exit

Under [Personal information] interface, select “Exit” to return to [Menu] interface.

| Personal Information | |
|----------------------|--------|
| Gender | FEMALE |
| Age | 20 |
| Height / cm | 160 |
| Weight / kg | 50 |
| Nation | ERS |
| Smoker | NO |
| Drug | NO |

Figure 11

| Personal Information | |
|----------------------|-----|
| Age | 20 |
| Height / cm | 160 |
| Weight / kg | 50 |
| Nation | ERS |
| Smoker | NO |
| Drug | NO |
| Exit | |

Figure 12

b. DATA MANAGEMENT

Under [Menu] interface, select “Data management” to enter [Data management] interface, as shown in Fig.13. Under the interface, functions such as review, view trend curve, delete data, denote value setting can be realized.

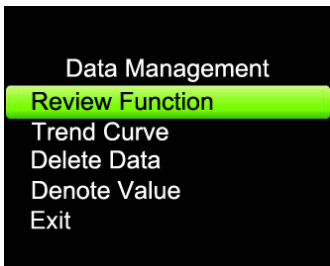


Figure 13 Data management interface

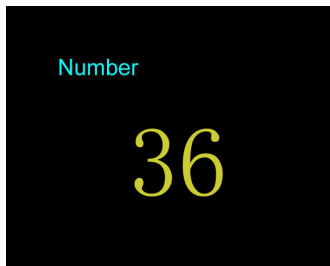


Figure 14 Case selection interface

1. Review function

Under [Data management] interface, select “Review function” to enter [Case selection] interface as shown in Fig.14, press “Up” or “Down” key (long press is available) to change case number, then press “Confirm” key, the device will enter [Main interface] and display history data on it. Under [Main interface], press “Up” or “Down” key continuously can review data in adjacent case number, press “Confirm” key to return to [Menu] interface.

2. Trend curve

Under [Data management] interface, select “Trend Curve” to enter [Trend curve selection] interface as shown in Fig.15. Select the determinant parameter, then press “Confirm” key to enter [Trend curve display] as shown in Fig.15. The curve is a summary of stored data for selected parameter. It displays the change trend in form of visual image, which is convenient for comparison. If the data is too much, press “Up” or “Down” key to browse all data trend curves orderly. Press “Confirm” key to return to [Data management] interface.

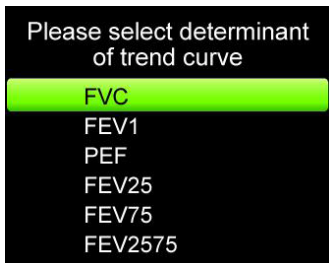


Figure 15 Trend curve selection interface

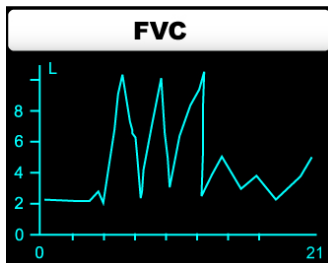


Figure 16 Trend curve display interface

3. Delete data

Under [Data management] interface, select “Delete data” to enter [Delete data] interface as shown in Fig.17. If choose “Yes”, the screen displays “waiting...”, all data will be deleted, then return to [Data management] interface. If choose “No”, it will return to [Data management] interface directly.

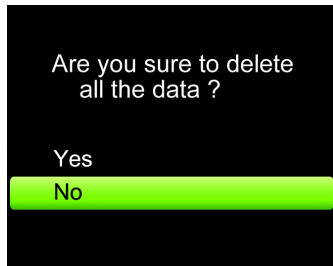


Figure 17 Delete data interface

4. Denote value

Under [Data management] interface, select “Denote value” to enter [Denote value setting] interface as shown in Fig.18. Select one parameter to decide the denote value, after that, it will automatically return to [Data management] interface.

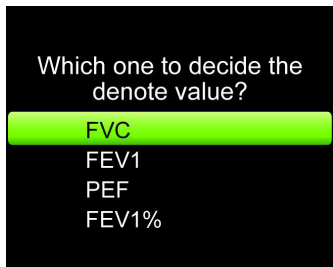


Figure 18 Denote value setting interface

5. Exit

Under [Data management], select “Exit” to return to [Menu] interface.

c. SETTINGS

Under [Menu] interface, select “Settings” to enter [Settings] interface as shown in Fig.19. Under this interface, settings of language, Bluetooth on/off, time and calibration, and view device information can be realized.

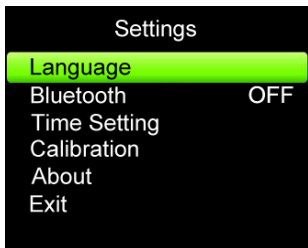


Figure 19 Setting interface



Figure 20 Language setting interface

1. Language setting

Under [Settings] interface, select “Language” to enter [Language setting] interface as shown in Fig.20. Select “English”, the device language will be English, select “中文”, the device language will be Chinese, after selected, it will automatically return to [Settings] interface

2. Bluetooth

Move selection toolbar to “Bluetooth”, press “Confirm” key to select “ON” or “OFF” that can turn on or off the Bluetooth module (If there is no Bluetooth module in the device, the operation is invalid).

3. Time setting

Under [Settings] interface, select “Time” to enter [Time setting] interface as shown in Fig.21. Select “Minute” to enter [Minute setting] interface, as shown in Fig.22. Press “Up” or “Down” key to change the value (long pressing is available), then press “Confirm” key to return to [Time setting] interface.

The operation of “Hour”, “Day”, “Month”, “Year” is similar to the “Minute”. The “Week” will be calculated according to “Year”, “Month” and “Day”, which does not need to set manually. Then select “Exit” to return to [Settings] interface.



Figure 21 Time setting interface

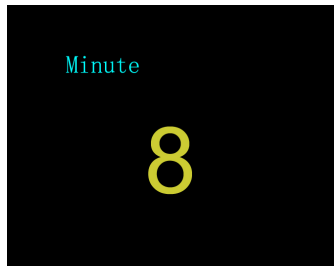


Figure 22 Minute setting interface

4. Calibration

Under [Settings] interface, select “Calibration” to enter [Calibration setting] interface as shown in Fig.23. Select 2L or 3L based on the volume of syringe, then enter to [Calibrate] interface as shown in Fig.24.



Figure 23 Calibration setting interface

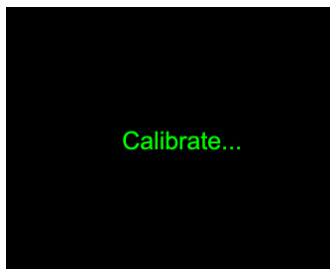



Figure 24 Calibrate interface

Under [Calibrate] interface, push the syringe once, the device will display “REPEAT”, then push the syringe once again. After twice correct continuous operation, the calibrating will be succeed, and the device will display “OK!”. Finally the interface will jump to the former interface before calibration (The former interface: If the device is calibrated after measurement completed, it will return to [Settings] interface; if calibrated before measurement completed, it will return to [Testing] interface.).

If the device displays “Error! Please repeat”, it indicates something wrong with the operation, please repeat the calibrating until succeeded. If the device displays “Select right volume”, please confirm whether the volume of syringe and calibration selection is accordant, then repeat the calibrating until succeeded. If you need to stop calibrating, just press the “Confirm” key to exit to the former interface before calibration.

Under [Calibration setting] interface, select “Adjust” to enter [Adjusting] interface, as shown in Fig.25. Press “Up” or “Down” key to change the value (long pressing is available), then press “Confirm” key to return to [Adjusting confirm] interface, as shown in Fig.26. Selecting “Yes” will save adjusted value, selecting “No” will cancel the setting, then the device will return to [Calibration setting] interface.



 **Note:** The value determines the accuracy of measurement, please do NOT change it randomly. After the turbine has been replaced, calibration shall be applied for inputting parameters of new turbine, which guarantees the accuracy of measurement after turbine replaced.

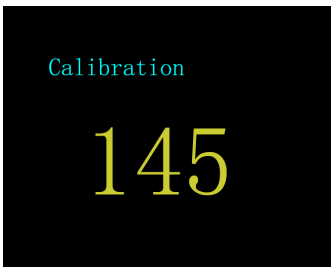


Figure 25 Adjusting interface

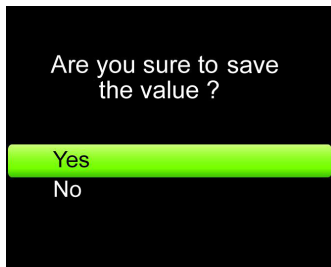


Figure 26 Adjusting confirm interface

Under [Calibration setting] interface, select "Exit" to return to [Settings] interface.

5. About device

Under [Settings] interface, select "About" to enter [About] interface. User can view device name and software version. Press "Confirm" key to return to [Settings] interface.

6. Exit

Under [Settings] interface, select "Exit" to return to [Menu] interface.

d. POWER OFF

Under [Menu] interface, select “Power off”, the device will shut down.

Note: If there is no operation within 1 minute, the device will power off automatically.

e. EXIT

Under [Menu] interface, select “Exit” to return to [Main interface]. If the measurement is not completed before enter [Main interface], it will return to [Testing] interface.

6.1.5 Repeated measure

Measurement of the device is repeatable. Long press “Repeated measure” key to enter [Testing] interface. When the memory is full, it will display [Memory full] interface as shown in Fig.27. If you select “Yes”, it will enter [Delete data] interface; if you select “No”, it will enter [Menu] interface.

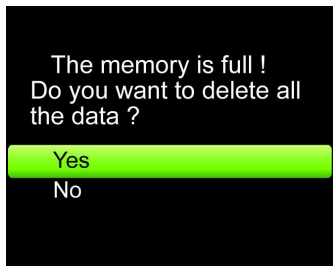



Figure 27

6.1.6 Charge

There are two kinds of charging methods

- 1) Connect the device with computer by data line then the device should be under charging state.
- 2) Connect the device with power supply by power adapter, then the device should be under charging state.

 For device charging, connect it with the power where easy to be cut off, after charging completed, unplug the power adapter to cut off from power.

6.1.7 Upload Data

Install the PC software in the computer, then the following figure will appear after completing.



Figure 28

- 1) Connect the device with computer by data line, double press the icon to open the PC software procedure.
- 2) Press the corresponding key to achieve upload data, delete case, print information, background, select language, switch PDF format, set the testee information etc.
- 3) Press "Exit" to exit the software, unplug the data line from the computer to achieve uploading.

6.2 Attention

- 🔔 Please check the device before using, and confirm that it can work normally.
- 🔔 Rechargeable lithium battery.
- 🔔 It is recommended that the device should be measured in room.
- 🔔 Excessive ambient light may affect measurement accuracy. It includes fluorescent lamp, dual ruby light, infrared heater, direct sunlight and etc.
- 🔔 Intense activity of the subject or extreme electrosurgical interference may also affect the accuracy.
- 🔔 Please clean and disinfect the device after using according to the User Manual (7.1).

Chapter 7

MAINTENANCE, TRANSPORTATION AND STORAGE

7.1 Cleaning and Disinfection

Using medical alcohol to wipe the device for disinfecting, nature dry or clean it with clean soft cloth. It's necessary to clean the turbine periodically for accuracy, keep the diaphaneity of the lucency part, and keep it away sundries (such as hair or lesser sediment). Immerse the turbine in disinfectant after use, clean it with clean water and dry standing vertically after soaked a few minutes (but don't make the turbine rinsed with water directly), this type doesn't bring pollution to environment. (Note: The disinfectant is 75% alcohol).

7.2 Maintenance

- 1) Please clean and disinfect the device before using according to the User Manual (7.1).
- 2) Please recharge the battery when the screen shows low-power (the battery power is).
- 3) Recharge the battery soon after the over-discharge. The device should be recharged every six months when it is not regular used. It can extend the battery life following this guidance. If the battery is broken, DO NOT try to maintain it by yourself, please contact us or the local service center.
- 4) The device needs to be calibrated once a year (or according to the calibrating program of hospital). It also can be performed at the state-appointed agent or just contact us for calibration.



7.3 Transportation and Storage

- 1) The packed device can be transported by ordinary conveyance or according to transport contract. The device can not be transported mixed with toxic, harmful, corrosive material.
- 2) The packed device should be stored in room with no corrosive gases and good ventilation. Temperature: $-40^{\circ}\text{C}\sim+55^{\circ}\text{C}$; Relative Humidity: $\leq 95\%$.

Chapter 8 TROUBLESHOOTING

| Trouble | Possible Reason | Solution |
|---|--|---|
| The device can't finish measurement for a long time, and the data can't be displayed. | The start speed is too low, the device does not measure. | Remeasure according to the user manual. |
| | The malfunction of the device. | Press "Repeated Measure" key to remeasure, or power off to restart. |
| The figure is wrong and unorderly. | The power turned off abnormally. | Delete the current case and remeasure. |
| | Operation is wrong. | Operate normally according to the user manual. |
| | The malfunction of the device. | Please contact the local service center. |
| The device can not be powered on. | Low battery or no power. | Please charge the battery. |
| | The malfunction of the device. | Please contact the local service center. |

| | | |
|--|--|--|
| The display disappears suddenly. | The device is set to automatic power off when there is no operation in one minute. | Normal. |
| | The battery is drained away or almost drained away. | Please charge the battery. |
| The device can not be used for full time after charge. | The battery is not full charged. | Please recharge the battery. |
| | The battery is broken. | Please contact the local service center. |
| The battery can not be full charged even after 10 hours charging time. | The battery is broken. | Please contact the local service center. |

Chapter 9

KEY OF SYMBOLS

| Symbol | Meanings |
|--------------|--|
| | Follow instructions for use |
| | Medical Device complies with Directive 93/42/EEC |
| | WEEE disposal |
| | Type BF applied part |
| | Full-power |
| | Low-power |
| Error | Measured value goes beyond the limits |
| | Status indicator bar |
| | Atmospheric pressure limitation |
| | Humidity limitation |

| Symbol | Meanings |
|---------------|---|
| | Store between -40 and 55°C |
| | Fragile, handle with care |
| | Keep in a cool, dry place |
| | This way up |
| | Date of manufacture |
| REF | Product code |
| LOT | Lot number |
| SN | Serial number |
| | Caution: read instructions (warnings) carefully |
| | Manufacturer |
| EC REP | Authorized representative in the European community |

Chapter 10

PARAMETER INTRODUCTION

| Measured parameters | | |
|----------------------------|---|-------------|
| Parameter | Description | Unit |
| FVC | Forced vital capacity | L |
| FEV1 | Forced Expired Volume in one second | L |
| PEF | Peak expiratory flow | L/s |
| FEV1 | $FEV1/FVC \times 100$ | % |
| FEF25 | 25% flow of the FVC | L/s |
| FEF2575 | Average flow between 25% and 75% of the FVC | L/s |
| FEF75 | 75% flow of the FVC | L/s |

Appendix I

Guidance and manufacturer's declaration – electromagnetic emissions- for spirometer

Guidance and manufacturer's declaration – electromagnetic emission

The spirometer (SP10) is intended for use in the electromagnetic environment specified below. The customer of the user of the spirometer (SP10) should assure that it is used in such an environment.

| Emission test | Compliance | Electromagnetic environment – guidance |
|-----------------------|-------------------|---|
| RF emissions CISPR 11 | Group 1 | The spirometer (SP10) uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment. |
| RF emission CISPR 11 | Class B | The spirometer (SP10) is suitable for use in all establishments, other than domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes. |

Guidance and manufacture's declaration – electromagnetic immunity – for spirometer

Guidance and manufacture's declaration – electromagnetic immunity

The spirometer (SP10) is intended for use in the electromagnetic environment specified below. The customer or the user of SP10 should assure that it is used in such an environment.

| Immunity test | IEC 60601 test level | Compliance level | Electromagnetic environment - guidance |
|---|----------------------------|----------------------------|--|
| Electrostatic discharge (ESD) IEC 61000-4-2 | ±6 kV contact ±8 kV air | ±6 kV contact ±8 kV air | Floors should be wood, concrete or ceramic tile. If floor are covered with synthetic material, the relative humidity should be at least 30%. |
| Power frequency (50/60Hz) magnetic field IEC61000-4-8 | 3A/m | 3A/m | Power frequency magnetic fields Should be at levels characteristic of a typical location in a typical commercial or hospital environment. |




Guidance and manufacturer's declaration – electromagnetic immunity – for spirometer (SP10) that are not LIFE-SUPPORTING

Guidance and manufacturer's declaration – electromagnetic immunity

The spirometer (SP10) is intended for use in the electromagnetic environment specified below. The customer or the user of spirometer (SP10) should assure that it is used in such an environment.

| Immunity test | IEC 60601 test level | Compliance level | Electromagnetic environment - guidance |
|------------------------------|-------------------------------|------------------|--|
| Radiated RF IEC 61000-4-3 | 3 V/m 80 MHz to 2.5 GHz | 3 V/m | <p>Portable and mobile RF communications equipment should be used no closer to any part of the spirometer (SP10), including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter.</p> <p>Recommended separation distance</p> $d = 1.17 \sqrt{P} \quad 80 \text{ MHz to } 800 \text{ MHz}$ $d = 2.33 \sqrt{P} \quad 800 \text{ MHz to } 2.5 \text{ GHz}$ <p>Where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in metres (m).</p> |

| | | | |
|--|--|--|---|
| | | | <p>Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey,^a should be less than the compliance level in each frequency range.^b Interference may occur in the vicinity of equipment marked with the following symbol:</p>  |
| <p>NOTE 1 At 80 MHz and 800 MHz, the higher frequency range applies. NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.</p> | | | |
| <p>a. Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the SP10 is used exceeds the applicable RF compliance level above, the SP10 should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as reorienting or relocating the SP10. b. Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3 V/m.</p> | | | |



Recommended separation distances between portable and mobile RF communications equipment and the spirometer (SP10)

Recommended separation distances between portable and mobile RF communications equipment and the spirometer (SP10)

The spirometer (SP10) is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the spirometer (SP10) can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the spirometer (SP10) as recommended below, according to the maximum output power of the communications equipment.

| Rated maximum output power of transmitter (W) | Separation distance according to frequency of transmitter (m) | | |
|---|---|--|---|
| | 150 kHz to 80 MHz $d = 1.17 \sqrt{P}$ | 80 MHz to 800 MHz $d = 1.17 \sqrt{P}$ | 800 MHz to 2.5 GHz $d = 2.33 \sqrt{P}$ |
| 0,01 | 0,12 | 0,12 | 0,23 |
| 0,1 | 0,37 | 0,37 | 0,74 |
| 1 | 1,17 | 1,17 | 2,33 |
| 10 | 3,70 | 3,70 | 7,37 |
| 100 | 11,70 | 11,70 | 23,30 |

For transmitters rated at a maximum output power not listed above, the recommended separation distance d in metres (m) can be estimated using the equation applicable to the frequency of the transmitter, where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

NOTE 1 At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.

NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.



Disposal: *The product must not be disposed of along with other domestic waste. The users must dispose of this equipment by bringing it to a specific recycling point for electric and electronic equipment. For further information on recycling points contact the local authorities, the local recycling center or the shop where the product was purchased. If the equipment is not disposed of correctly, fines or penalties may be applied in accordance with the national legislation and regulations.*

GIMA WARRANTY CONDITIONS

Congratulations for purchasing a GIMA product. This product meets high qualitative standards both as regards the material and the production.

The warranty is valid for 12 months from the date of supply of GIMA.

During the period of validity of the warranty, GIMA will repair and/or replace free of charge all the defected parts due to production reasons.

Labor costs and personnel traveling expenses and packaging not included.

All components subject to wear are not included in the warranty.

The repair or replacement performed during the warranty period shall not extend the warranty. The warranty is void in the following cases: repairs performed by unauthorized personnel or with non-original spare parts, defects caused by negligence or incorrect use. GIMA cannot be held responsible for malfunctioning on electronic devices or software due to outside agents such as: voltage changes, electro-magnetic fields, radio interferences, etc.

The warranty is void if the above regulations are not observed and if the serial code (if available) has been removed, cancelled or changed.

The defected products must be returned only to the dealer the product was purchased from. Products sent to GIMA will be rejected.





